

10-27-00

A

Case Docket No. PHF 99,595

COMMISSIONER FOR PATENTS, Washington, D.C. 20231

Enclosed for filing is the patent application of Inventor(s):
RAOUL FLORENT LUCILE GOUBET

For: IMAGE PROCESSING METHOD, SYSTEM AND APPARATUS FOR NOISE REDUCTION IN AN IMAGE
SEQUENCE REPRESENTING A THREADLIKE STRUCTURE

10/26/00
09/697389
PTO
U.S.

ENCLOSED ARE:

- ☒ Associate Power of Attorney;
- ☒ Information Disclosure Statement, Form PTO-1449 and copies of documents listed therein;
- ☒ Preliminary Amendment;
- ☒ Specification (16 Pages of Specification, Claims, & Abstract);
- ☒ Declaration and Power of Attorney:
(2 Pages of a [] fully executed [X] unsigned Declaration);
- ☒ Drawing (3 sheets of [] informal [X] formal sheets);
- ☐ Certified copy of application Serial No. ;
- ☒ Authorization Pursuant to 37 CFR 1.136(a)(3)
- ☒ Other: RELATED CASES;
- ☐ Assignment to

FEE COMPUTATION

CLAIMS AS FILED				
FOR	NUMBER FILED	NUMBER EXTRA	RATE	BASIC FEE - \$690.00
Total Claims	11- 20 =	0	X \$18 =	0.00
Independent Claims	1 - 3 =	0	X \$80 =	0.00
Multiple Dependent Claims, if any			\$270 =	0.00
TOTAL FILING FEE			=	\$710.00

Please charge Deposit Account No. 14-1270 in the amount of the total filing fee indicated above, plus any deficiencies. The Commissioner is also hereby authorized to charge any other fees which may be required, except the issue fee, or credit any overpayment to Account No. 14-1270.

[] Amend the specification by inserting before the first line the sentence: This is a continuation-in-part of application Serial No. , filed .

John F. Vodopia, Reg. 36,299
Attorney
914-333-9627

CERTIFICATE OF MAILING

[X] Express Mail Mailing Label No. EL456215149

Date of Deposit October 26, 2000

I hereby certify that this paper and fee is being deposited with the United States Postal Service "Express Mail Post Office to Addressee" service under 37 CFR 1.10 on the date indicated above and is addressed to the Commissioner for Patents, Washington, D.C. 20231

Valerie T. Deas

Valerie T. Deas

Name

Signature

Send correspondence and papers to Corporate Patent Counsel
U.S. Philips Corporation, 580 White Plains Road, Tarrytown, New York 10591

F:\WPDOCS\vo\phf99595.app.doc

10/26/00
10/26/00
PTO
U.S.

	1990	1991	1992	1993	1994	1995	1996	1997	1998	1999	2000	2001	2002	2003	2004	2005	2006	2007	2008	2009	2010	2011	2012	2013	2014	2015	2016	2017	2018	2019	2020	2021	2022	2023	2024	2025	2026	2027	2028	2029	2030	2031	2032	2033	2034	2035	2036	2037	2038	2039	2040	2041	2042	2043	2044	2045	2046	2047	2048	2049	2050	2051	2052	2053	2054	2055	2056	2057	2058	2059	2060	2061	2062	2063	2064	2065	2066	2067	2068	2069	2070	2071	2072	2073	2074	2075	2076	2077	2078	2079	2080	2081	2082	2083	2084	2085	2086	2087	2088	2089	2090	2091	2092	2093	2094	2095	2096	2097	2098	2099	2100	2101	2102	2103	2104	2105	2106	2107	2108	2109	2110	2111	2112	2113	2114	2115	2116	2117	2118	2119	2120	2121	2122	2123	2124	2125	2126	2127	2128	2129	2130	2131	2132	2133	2134	2135	2136	2137	2138	2139	2140	2141	2142	2143	2144	2145	2146	2147	2148	2149	2150	2151	2152	2153	2154	2155	2156	2157	2158	2159	2160	2161	2162	2163	2164	2165	2166	2167	2168	2169	2170	2171	2172	2173	2174	2175	2176	2177	2178	2179	2180	2181	2182	2183	2184	2185	2186	2187	2188	2189	2190	2191	2192	2193	2194	2195	2196	2197	2198	2199	2200	2201	2202	2203	2204	2205	2206	2207	2208	2209	2210	2211	2212	2213	2214	2215	2216	2217	2218	2219	2220	2221	2222	2223	2224	2225	2226	2227	2228	2229	2230	2231	2232	2233	2234	2235	2236	2237	2238	2239	2240	2241	2242	2243	2244	2245	2246	2247	2248	2249	2250	2251	2252	2253	2254	2255	2256	2257	2258	2259	2260	2261	2262	2263	2264	2265	2266	2267	2268	2269	2270	2271	2272	2273	2274	2275	2276	2277	2278	2279	2280	2281	2282	2283	2284	2285	2286	2287	2288	2289	2290	2291	2292	2293	2294	2295	2296	2297	2298	2299	2300	2301	2302	2303	2304	2305	2306	2307	2308	2309	2310	2311	2312	2313	2314	2315	2316	2317	2318	2319	2320	2321	2322	2323	2324	2325	2326	2327	2328	2329	2330	2331	2332	2333	2334	2335	2336	2337	2338	2339	2340	2341	2342	2343	2344	2345	2346	2347	2348	2349	2350	2351	2352	2353	2354	2355	2356	2357	2358	2359	2360	2361	2362	2363	2364	2365	2366	2367	2368	2369	2370	2371	2372	2373	2374	2375	2376	2377	2378	2379	2380	2381	2382	2383	2384	2385	2386	2387	2388	2389	2390	2391	2392	2393	2394	2395	2396	2397	2398	2399	2400	2401	2402	2403	2404	2405	2406	2407	2408	2409	2410	2411	2412	2413	2414	2415	2416	2417	2418	2419	2420	2421	2422	2423	2424	2425	2426	2427	2428	2429	2430	2431	2432	2433	2434	2435	2436	2437	2438	2439	2440	2441	2442	2
--	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	---

•

2

PRELIMINARY AMENDMENT

Sir:

Prior to calculation of the filing fee and examination, please amend the above-identified application as follows:

IN THE SPECIFICATION

Page 1, before line 1, insert the following heading:

--BACKGROUND OF THE INVENTION--;

before line 9, insert the following heading:

--SUMMARY OF THE INVENTION--;

line 22, change "It results that" to --By use of the
method,--;

line 25, change "provides" to --provide--;

Page 2, line 11, change "to operate" to --direct--;

line 12, delete "the propagation of"; change "for a" to
--thereby--; delete "to be made to";

line 19, change "as claimed in Claim 1." to --for noise
' filtering an image sequence representing a
threadlike structure on a background, including
an acquisition of point data in first and
second sequence images and an estimation of the
corresponding filtered point data for
constructing a filtered second image, the point
data being the intensities associated to co-
ordinates of image points, said method
comprising, performed in each sequence image,
steps of: extracting the threadlike structure
points, forming strings from said extracted
points, temporally filtering the data of the
points located outside the strings denoted
background points, spatially filtering the data
of the string points, and constructing the
filtered second image data by performing an
insertion of the spatially filtered data of the
string points into the temporally filtered data
of the background points.--;

line 22, change "is further claims in claim 11" to
--includes a computer program product
comprising a set of instruction for carrying

out a method as claimed in claim 1--;

line 23, ' change "is " to -- 'as claimed in claim 6,
including an enhancement operation performed on
spatially filtered string point data,
comprising steps of: selecting string points
[A(i,j)] using the list of the control signal
[St(i,j)], enhancing the string point data with
respect to their local environment, and
constructing a filtered second image data by
performing an insertion of the enhanced
spatially filtered data of the string points
into the temporally filtered data of the
background points, controlled by the binary
control signal--;

line 24, delete "claimed in claim 12;

before line 27, insert the following heading:

--BRIEF DESCRIPTION OF THE DRAWINGS--;

line 30, after "background;" begin a new paragraph;

line 31, after "operation;" begin a new paragraph;

line 32, after "branches;" begin a new paragraph;

Page 3, line 2, after "1" insert --;-- (semicolon); and after
"and" (2nd occurrence) begin a new paragraph;
line 22, change "denoted" to --denoting--;

between lines 30 and 31, insert the following heading:

' --DESCRIPTION OF THE PREFERRED EMBODIMENTS--;
and

Page 4, line 18, delete "of";

Page 5, line 31, after "point" (last occurrence) insert --or--.

IN THE CLAIMS

Please amend claims 1, 7, 8, 9 10 and 11 as follows:

Claim 1, line 7, after "points," began a new paragraph;
line 8, after "points, (1st occurrence) begin a new
paragraph;
line 9, after "points," (1st occurrence) being a new
paragraph.

Claim 7, line 1, change "Claims 5 or 6" to --claim 5--.

Claim 8, line 1, change "one of the preceding Claims" to
--claim 1--.

Claim 9, line 3, change "any of Claims 1 to 8" to --claim 1--.

Claim 10, line 2, after "9" insert --,-- (comma).

Claim 11, line 1, ' change "instruction" to '--instructions--;
line 2, change "one of claims 1 to 8" to --claim 1--.

Please add the following new claim 12:

12. A method as claimed in claim 6, including an enhancement operation performed on spatially filtered string point data, comprising steps of :

selecting string points [A(i,j)] using the list of the control signal [St(i,j)],

enhancing the string point data with respect to their local environment,

and constructing a filtered second image data by performing an insertion of the enhanced spatially filtered data of the string points into the temporally filtered data of the background points, controlled by the binary control signal.

IN THE ABSTRACT

Page 16, before line 1, delete in its entirety and substitute the following heading: --ABSTRACT OF THE DISCLOSURE--;
line 4, change "image said method comprising," to
--image. The method is--;

line 5, change ", steps of." to --and includes--;
line 6, ' continue on previous line;
change "said" to --the--;
line 9, continue on previous line;
lines 12-15; delete in their entirety.

REMARKS

This Preliminary Amendment is submitted to place the application in proper U.S. format. Entry is respectfully requested.

Respectfully submitted,


By 
Edward W. Goodman, Reg. 28,613
Attorney
(914) 333-9611

Image processing method, system and apparatus for noise reduction in an image sequence representing a threadlike structure

The invention relates to an image processing method for noise reduction in a sequence of noisy images representing a threadlike structure on a background. The invention particularly relates to noise reduction method applied to a sequence of medical X-ray fluoroscopy images representing a catheter guide-wire. The invention also relates to a system
5 for carrying out this method and to an examination apparatus having means for image processing. The invention is applied to the medical imaging.

An image processing system for filtering X-ray fluoroscopic image sequence
10 is already known of a US patent N°5809105. This document discloses means for acquiring one image by passing X-rays through a subject, said image comprising an array of pixel values, means for receiving the image and producing a mask therefrom which distinguishes the pixel values that correspond to structural features in the image from the pixel values that correspond to background and means being responsive to the mask for selectively filtering
15 the pixel values in the image that correspond to background. The means for filtering the background pixel values include a Poisson filter which is spatial filter. So, the mask is used to select the background pixels for filtering the background noise while enabling the structural pixels to pass unfiltered to the display.

20 This known method does not provide means to detect object motion in an image sequence. It results that it may be difficult to filter the background by applying the mask without degradation of said structural features, especially if they represent a very thin threadlike structure. The mask may cover up said threadlike structure when a non-detected
25 swift motion occurs. Besides, this known method does not provides means to eliminate phantom artifacts. Furthermore, this known method does not provide means for noise filtering the object pixels themselves. This is a drawback because the boundaries of a thin threadlike structure may be blurred by noise, which makes said threadlike structure difficult to localize, whereas the central points of the threadlike structure may be sputtering due to

noise, which makes this threadlike structure difficult to visualize, even when the background has been noise filtered. Moreover, the known method does not permit enhancement of the structural features with respect to the background. This is a drawback when the thin threadlike structure presents little contrast with respect to a noisy cluttered background.

5 In cardiology, a sequence of images may be formed of images representing blood vessels called arteriogram images used to visualize in real time medical procedures of introducing a catheter in a vessel. Such medical procedures deeply rely on the correct visibility of a metallic guide-wire, which is introduced in the vessel for guiding the catheter. These fluoroscopic digital images are noisy because they are formed with a low level of X-
10 rays. It is very important to improve considerably the guide-wire visualization in image sequences formed in the X-ray fluoroscopic mode in order to help the practitioner to operate the propagation of the catheter in the arteries for avoiding damage to be made to said arteries during this operation.

The invention aims at providing an image processing method to be applied to a
15 noisy image sequence representing a threadlike structure on a background, at improving the background noise reduction without degradation of said threadlike structure, at eliminating the phantom artifacts and at noise filtering and enhancing the threadlike structure in real time, for example at a rate of about 25 images per second.

These aims are reached by an image processing method as claimed in Claim 1.

20 Advantages of this method are that the object of interest localization is much more accurate, while the processing method is carried out in real time.

A system to carry out said method is further claimed in claim 11, and an examination apparatus with a system and means for carrying out the processing method is claimed in claim 12.

25 The invention is described thereafter in detail in reference to diagrammatic figures, wherein :

FIG.1 is a functional block diagram illustrating the steps of the method ;

30 FIG.2A shows an original image of a guide-wire on a background; FIG.2B shows an image of guide-wire extracted pixels supplied by the GWE operation; FIG.2C shows an image of strings with branches; FIG.2D shows an image of an independent string;

FIG.3 illustrate the step of local enhancement of the string point intensities;

FIG.4A is a functional block diagram illustrating an examination apparatus having a system and means for carrying out the method of FIG.1 and FIG.4B illustrates an X-ray apparatus for providing image data to a processing system.

5

The invention relates to an image processing method for noise filtering an image sequence representing a threadlike structure, possibly moving on a background, including an acquisition of the point data in first and second sequence images and an estimation of the corresponding filtered point data to reconstruct a noise filtered second image. By threadlike structure, one understands an elongated shaped object, having a transversal dimension of 1 to 10 pixels, possibly 1 to 3 pixels, in a digital image. The point data are the intensities and co-ordinates of the points in the images.

In an example described hereafter, the invention particularly relates to a noise reduction method applied to a sequence of medical X-ray fluoroscopic noisy images representing a threadlike structure that is a catheter guide-wire on a cluttered background. The image processing method aims at reconstructing an improved sequence of images where the point intensities of the guide-wire are noise filtered and enhanced with respect to a filtered background. One problem lies in the selection of the points that must be both filtered and enhanced as guide-wire points, or that must be filtered as background points, in the sequence images. This problem is solved by an image processing method comprising steps of extracting the guide-wire points, forming strings from said extracted guide-wire points, temporally filtering the points located outside the strings, denoted background points, spatially filtering the points located on the strings denoted guide-wire points and inserting the spatially filtered guide-wire points in the image of the temporally filtered background points. An other problem lies in the elimination of phantom artifacts. This problem is solved by processing a sequence of two images and by selecting for insertion the guide-wire points that have been located on a string in at least one of the two images. An other problem lies in the lack of contrast of the original images. This problem is solved by applying local intensity enhancement on the spatially filtered guide-wire string points and inserting the resulting enhanced guide-wire string points in the image of the temporally filtered background points.

Referring to FIG.1, the method comprises the main operations of:

acquisition 100 of digital intensity signals X_t-1 or X_t of an arteriogram image representing a guide-wire GW on a background BG, as shown in FIG.2A;

extraction 10 of the guide-wire points from the arteriogram image, meaning detection and location of the guide-wire points, providing a binary signal $Mt-1$, Mt of detected guide-wire points associated to their co-ordinates i, j , as shown in FIG.2B;

string formation 90 from the extracted guide-wire points for providing a string signal $St(i, j)$ of numbered string points, with their co-ordinates i, j , as shown in FIG.2C;

insertion 40 of spatially noise filtered guide-wire intensities of points located on the strings in an image of temporally recursive noise filtered intensities of points not located on the strings, referred to as background points;

spatial filtering 60 of the intensities of the numbered guide-wire points located on the strings, considered as temporal samples;

local enhancement 70 of the spatially filtered guide-wire string point intensities;

and insertion 80 of the enhanced spatially filtered guide-wire point intensities located on the strings in the already temporally filtered background image for providing final filtered samples denoted $OUFt$ representing the final filtered image.

This method also comprises a step 50 of elimination of phantom artifacts, which is performed using two successive arteriogram images in a sequence. The use of two images also permits of performing temporally recursive filtering for noise filtering the background.

As described in more detail hereafter, the following method is preferably carried out using two successive images of an image sequence, including a first image referred to as causal image acquired at a first instant $t-1$, and a second image referred to as present image acquired at a second instant t . This method performs the processing of the image points according to a standard scanning of the images so as to filter each current point one after the other. The co-ordinates of the current point in the images are denoted i, j and the intensity values, referred to as samples, at this location i, j in the causal and present original images, are respectively denoted $Xt-1$, Xt . This method is performed in real time, that is to say at a rate of about 25 images per second.

In this image processing method, the filtering of the background is preferably carried out using a temporal recursive adaptive filter. Temporal filters are generally known as giving the best filtering results in image sequences representing objects without motion. In image sequences representing objects with motion, temporal recursive filter that are made adaptive to motion may be used. However, in that case, complete moving-detail preservation is virtually impossible. So, using a temporal recursive filter in an image sequence comprising

a moving object as thin as said guide-wire may expose so thin a structure to some amount of degradation. In fact, a temporal recursive filter relies on pixel-wise fuzzy decisions regarding the motion occurrence between consecutive images. Since these decisions are fuzzy and since X-ray fluoroscopic images are usually very noisy, a temporal filter fails to completely
 5 preserve weakly contrasted moving objects because it fails to reach certainty about the occurrence of motion. It is the reason why, according to the present method, the guide-wire points are extracted and then these guide-wire points are not temporally filtered. Instead, the extracted guide-wire points are processed in order to be spatially filtered.

In reference to FIG.2A, the guide-wire points are extracted in one image at a
 10 time, on a purely spatial basis, that is, regardless of its motion content. To that end, each original image is first scanned in order to determine whether the current point pertains to the image background BG or to the guide-wire GW. Then each guide-wire point is extracted. In reference to FIG.2B, based on the extracted points, strings of points are formed in order to eliminate guide-wire boundary points and to keep guide-wire central points for further
 15 processing. In reference to FIG.1, a recursive temporal filtering RTPF is applied to those points that are not extracted as string points and thus are denoted background points, whereas a spatial filtering SPF1 is applied to those points that are extracted as guide-wire string points. So, at a string point location, which is a guide-wire point location, as the probability of movement is high, no temporal filtering is performed; instead, a spatial filtering is
 20 performed; whereas, at a non-string point location, which is regarded as a background point location, as the probability of movement is low, temporal filtering is allowed to be performed. FIG.1 shows diagrammatically the detailed steps of the processing method for noise reduction in the images of a sequence representing a moving guide-wire as described above. This method provides a final filtered sample denoted OUFt relative to each current
 25 point at a location i, j for reconstructing a filtered image at time t from the samples X_{t-1} , X_t of the causal and present images. These detailed steps are :

acquisition 100 of the samples X_{t-1} , X_t of the current point located at the co-ordinates i, j respectively in the causal and present images of the sequence;

guide-wire extraction 10 performed by an extraction module denoted GWE
 30 receiving at its input 1 said samples X_{t-1} , X_t , and providing at its output 56 respective binary samples M_{t-1} , M_t , which are either a data 1 for a current point that is a guide-wire point a data 0 for a current point that is not a guide-wire point, thus is regarded as a background point; associated to the binary data values M_{t-1} , M_t related to points, are the co-ordinates i, j

of said points; this provides an image denoted IM_t of the guide-wire points of intensity 1 represented on a background of intensity zero, at the instant t , as shown in FIG.2B;

string formation 90, which transforms the image IM_t of the extracted guide-wire points into strings of chained points also referred to as connected points; a string point
 5 pertains to a set of connected points, so as each string point has two connected neighbors, except the two end points of the string, which have each only one neighbor; the step of string formation 90 may provide several strings or strings having several branches, for example B1, B2, B3.... as represented on FIG.2C; in that last case, the points that are common to several branches are called multiple-points and have to be detected using an operation of point
 10 detection known of those skilled in the art; this operation of point detection is followed by an operation of branch separation at the location of the multiple-points and evaluation of the most probable strings denoted SWS; FIG.2D shows an example of such an image, denoted IS_t , at the instant t ; the output 91 of the string module 90 supplies a list $St(i, j)$ of connected points characterized by point running numbers 1, 2,...k,...n on the string SWS and by the co-
 15 ordinates i, j of said string point in the image IS_t , such as : i_1, j_1 ; i_2, j_2 ; ...; i_k, j_k ; ... i_n, j_n ; the string formation step may be carried out using morphological filters performing a thinning operation providing structures denoted skeletons of extracted points; then, these skeletons are the base of constitution of the string SWS;

spatial filtering 20 performed by a purely spatial filter module denoted SPF1,
 20 which receives at its input 2 the sample X_t of the present image, and provides at its output 40B a spatially filtered sample referred to as gate sample denoted G_t ; this spatial filtering operation is not compulsory : the original signal X_t may be used directly in the further step 40 instead of the gate signal G_t because spatial filtering will be performed in further steps of the image processing method; however said spatial filtering operation 20 is recommended in
 25 order to smooth the sample X_t , which in every case improves said method;

temporal filtering 30 performed by a temporal recursive filter module denoted TPRF, which receives at its input 4 said samples X_{t-1} , X_t of the causal and present images, and provides at its output 40A a temporally filtered sample denoted Y_t . This temporal filter is connected to a loop 49 providing a delay Δ , which receives at its input 40A the filtered
 30 sample Y_t and supplies at its output 47 a stored causal sample Y_{t-1} for the temporal filter TPRF to perform a recursive temporal filtering.

The string formation operation provides several advantages : The guide-wire is replaced by a string structure meaning that the blurred boundary points are now eliminated

and that only guide-wire central points are processed. This operation also provides the list signal $St(i,j)$ which is a control signal for the construction of the further filtered images.

The operations of string formation, spatial filtering and temporal filtering are performed in parallel. In an example of realization, the extracting module 10 denoted GWE, which performs the guide-wire point extraction, may comprise means or steps as those described in the EP0840252. The purely spatial filter 20 denoted SPF1, which provides the gate signal Gt from the original signal Xt , may be a spatial FMH (FIR-Median-Hybrid) filter such as described for example in the EP0755023. Such FMH filters show a good preserving ability for thin structures. A temporal recursive filter which can adapt itself to intensity discontinuities due to motion or noise peaks is already known, for example, of EP0751482. Such a filter is well adapted to be used in the present method.

Now, the processing method further comprises an insertion step 40 performed by a module denoted INSERTION 1, which issues at its output 40C, a signal $Zt(i,j)$ that depends on the location of the current point; said output signal $Zt(i,j)$ is:

either the gate sample $Gt(i, j)$, supplied by the spatial filter module SPF1 to the INSERTION 1 module input 40B, when the current point is determined as a string point by a signal control that is present at an input 40L of the INSERTION 1 module; in that case, the current point is in the list $St(i,j)$ at said location i, j at the present time t ,

or the temporally filtered sample $Yt(i,j)$, supplied by the temporal filter TPRF to INSERTION 1 module input 40A, when the current point is determined as a non-string point by the signal control at the input 40L of INSERTION 1 module; in that case, the current point is not in the list $St(i,j)$ at said location i, j at said present time t and is regarded as a background point.

The list signal $St(i,j)$ is a binary control signal 1 or 0 applied to the input 40L of the INSERTION 1 module 40. So, the INSERTION 1 module 40 inserts the intensities of the gate samples Gt at the locations i,j of the current points that are in the list $St(i,j)$ of guide-wire string points, and inserts the intensities of the temporally filtered samples Yt at the locations i,j of the current points that are not in the list $St(i,j)$ and that are non-string points, i. e. background points. In a general manner, the INSERTION 1 module 40 inserts the intensity image of the strings into the temporally filtered intensity image of the background.

The binary control signal at node 40L is provided by the binary output data of the string formation module 90 modified by a module 50 denoted PHE devised for eliminating phantom artifacts. The PHE module receives the binary string signals $St-1$, St at the node 56. The causal binary signal $St-1$, which is received first, is stored in a memory or a

delay 51 of the PHE module so as said causal sample $St-1$ may be available at node 58 at the present instant t at the same time as the present binary signal St is available at node 55. Then, nodes 55 and 58 constitutes the inputs of a logic OR 52 which delivers at the output 40L a binary signal equal to 1 every time that at least one of its inputs is equal to 1, or a binary signal equal to 0 only when both its inputs are equal to 0. This means that the output 40L of the PHE module 50 delivers a signal 0 corresponding to the presence of a non-string point, referred to as background point, uniquely when both causal and present binary signals $St-1$, St are themselves equal to 0, or a signal 1 corresponding to the presence of a guide-wire string point at the location i, j in all other cases, that is when at least one of the two binary samples $St-1$ and St is equal to 1 corresponding to the actual presence of a string point at the location i, j in at least one of the two images, the other image actually showing a non-string point, called background point.

The output 40L of the PHE module 50 constitutes the binary control signal of the INSERTION 1 module 40, which selects the gate sample Gt for further image processing when the PHE module outputs 1 corresponding to the actual presence of a string point whether in both the causal and present images or in only one of said images, or which selects the temporally filtered sample $Yt(i,j)$ for further image processing uniquely when the PHE module issues a signal 0 corresponding to the actual presence of non-string point, called background point, in both said images. Thus, the temporal filter is not allowed to provide a filtered sample $Yt(i,j)$ which is a smoothed combination of intensities at location i, j of samples at instants $t-1$ and t corresponding respectively to a non-string sample, denoted background sample, and to a string sample. It results that a string point which is present in i,j at the causal instant $t-1$ and which is no more present at the instant t is not allowed to show through the image reconstructed at the present instant t since the temporal filter is only allowed to provide filtered samples corresponding to non-string points, denoted background points. So, spatially filtered intensities $Gt(i,j)$, which are spatially filtered images of string points at the instant t , are inserted onto the phantom points, which were string points at instant $t-1$, whereas spatially filtered intensities $Gt(i,j)$, which are spatially filtered images of string points at the instant t , are inserted uniquely at the location of corresponding string points. The phantom artifacts due to temporal filtering are eliminated. Only spatially filtered images of guide-wire points, located on strings, are allowed to be inserted in the temporally filtered images of background points. The INSERTION 1 module 40 supplies at its output 40C the appropriate filtered sample $Gt(i,j)$ or $Yt(i,j)$ for forming the image signal $Zt(i,j)$.

The insertion operation 40 provides several advantages : In the temporal recursive process, the points belonging to the moving guide-wire at time t , which might have been partly impaired, are fruitfully replaced by their spatially filtered counterparts. Also in the temporal recursive process, the points corresponding to the locations that the moving guide-wire occupied in the previous image, at time $t-1$, which might have been corrupted by phantom artifacts, consisting in that the guide-wire points at time $t-1$ shows through the image at time t , are fruitfully replaced by their spatially filtered counterparts. The quantum noise of the background is reduced.

Now, the processing method comprises steps for noise filtering and enhancing the intensity of the guide-wire string points. For carrying out these steps, it is important to note that the list $St(i,j)$ is used as a control signal to select the string points in the processed images. Referring to FIG.1, these further processing steps are :

spatial filtering 60 performed on the image signal $Zt(i,j)$ using a spatial filter module SPF2, which receives the image sample $Zt(i,j)$ at its input 40C, the string signal $St(i,j)$, giving the co-ordinates i,j of the string points, at its control input 75 and which performs spatial filtering on the points belonging uniquely to the strings, string by string. In fact, the guide-wire string point intensities in the image $Zt(i,j)$ may be regarded as forming a temporal intensity signal denoted $Ht(i,j)$ constituted of the samples $Gt(i,j)$ considered between the start point corresponding to the first end point numbered 1 of the string SWS and the terminal point corresponding to the second end point numbered n of said string. Said temporal intensity signal $Ht(i,j)$ propagates from the start point to the end point. Each sample $Gt(i,j)$ of a guide-wire string has a number on said string, which is given by the string signal $St(i,j)$ and which is similar to a time co-ordinate in a standard temporal intensity signal. So, a recursive temporal filtering technique can be applied to the samples $Gt(i,j)$ of the strings in the image $Zt(i,j)$ in the same way as to a standard temporal intensity signal. To that end, the guide-wire string points are scanned along the string according to their point number on said string, which is delivered by the string signal $St(i,j)$ together with their co-ordinates in the image. The string point intensity is spatially filtered one point after the other in a causal direction, for example from the start point to the terminal point. Then said string point intensity can be further spatially filtered one point after the other in an anti-causal direction, for example from the terminal point to the start point in order to provide a recursive filtering with two passes, as in a temporal filtering technique. It has been found that two such passes in a causal and anti-causal direction provide a good noise filtering of the string point intensities in the $Zt(i,j)$ image signal. The SPF2 module issues a noise filtered image signal

Ut(i,j) at its output 61, which comprises the spatially filtered string point intensities denoted Ht(i,j) and the background temporally filtered intensities Yt(i,j). The guide-wire represented by said filtered string point intensities shows no more boundaries with unpleasant sputtering and is agreeably noise filtered with elimination of noise peaks.

To improve the visualization of the guide-wire in the difficult fluoroscopic images, the contrast of the guide-wire string point is further enhanced with respect to the background using an enhancement module 70 that receives the image signal Ut(i,j) with the noise filtered string point intensities Ht(i,j) at its input 61 and the string signal St(i,j) at its control input 91. This enhancement step 70 comprises operations of :

determination 71 a local neighborhood denoted V related to each point of a string, using a computation module denoted LN, which receives the string signal St(i,j) at its control input 76. As illustrated by FIG.3, a point A(ik,jk) of the string SWS is localized by its co-ordinates ik, jk given by the string signal St(i,j). Related to the string point A(ik,jk), a neighborhood Vk is determined; to that end the string direction is first evaluated by a mean value of the directions of said string SWS. Then the orthogonal direction SWO is evaluated from the string direction and the coordinates of about 3 points each side of the string SWS on said orthogonal direction SWO are determined, forming said neighborhood Vk;

estimation 72 of the local contrast at the point A(ik, jk) using a computation module denoted LC, which has an input 79 for the Vk neighborhood, an input 81 for the image signal Ut(i,j) and a control input 77 for the string signal St(i,j); as illustrated by FIG.3, a mean value of the intensities of the neighborhood points in Vk, which are non-string points and thus are background points, is estimated from the Ut(i,j) signal and denoted $\bar{U}(Vk)$; the intensity of the given point A(ik, jk), which is a string point, is estimated from Ut(i,j) and denoted U(ik,jk); the local contrast LC(ik,jk) is computed as the difference between the mean intensity on the neighborhood Vk and the intensity at the string point A(ik,jk) :

$$LC(ik,jk) = \bar{U}(Vk) - U(ik,jk) \quad (1)$$

amplification 73 of said local contrast LC(ik,jk) by a predetermined factor $C > 1$, using a multiplier module 73, which receives the local contrast LC(ik,jk) and which issues a signal Ft(ik,jk) related to said string point A(ik, jk) :

$$C. LC(ik,jk) = C \times \bar{U}(Vk) - C \times U(ik,jk) \quad (2)$$

$$C. LC(ik,jk) = \bar{U}(Vk) - Ft(ik,jk) \quad (3)$$

The signal Ft(ik,jk) is an enhanced intensity signal to be applied on the already spatially filtered string point A(ik,jk), whose calculation is based on the equations (2) and (3) :

$$Ft(ik,jk) = [C \times U(ik,jk)] - [(C - 1) \times \bar{U}(Vk)] \quad (4)$$

Now, the enhanced string point intensity signal, denoted $Ft(i,j)$, is calculated for all the points of the string SWS using formula (4) and is inserted into the image signal $Ut(i,j)$ at the coordinates of the string points given by the string signal $St(i,j)$. This operation is performed by a module 80, denoted INSERTION 2, which receives the image signal $Ut(i,j)$ at its input 80A, the enhanced string point signal $Ft(i,j)$ at its input 80B and the control signal $St(i,j)$, which is the string signal, at its control input 80L. The INSERTION 2 module 80 performs said insertion operation for issuing at its output 80C, a signal $OUFt(i,j)$ that depends on the location of the current point, which is :

either the enhanced spatially filtered sample $Ft(i,j)$ related uniquely to string point intensities, supplied by the enhancement module 70 to the INSERTION 2 module 80 at its input 80B, when the current point is determined a string point of the list $St(i,j)$ at said location i, j at the present time t , by said control signal applied at its input 80L :

$$OUFt(i,j) = Ft(i,j) = [C \times U(i,j)] - [(C - 1) \times \bar{U}(V)] \quad (5a)$$

or
$$OUFt(i,j) = Ft(i,j) = C.LC(i,j) - \bar{U}(V) \quad (5b)$$

or the temporally filtered sample $Yt(i,j)$, supplied by the INSERTION 1 module 40 to the INSERTION 2 module 80 at its input 80A, when the current point is determined as a non-string point by the control signal at the input 80L; the current point is not in the list $St(i,j)$ and is considered as a background point at said location i,j at said present time t .

$$OUFt(i,j) = Yt(i,j) \quad (6)$$

So, the INSERTION 2 module inserts the enhanced spatially filtered intensities of the string points into the temporally filtered intensities of the background, which means that the insertion module inserts the spatially filtered image of the strings into the temporally filtered image of the background. This INSERTION 2 module issues an image signal $OUFt(i,j)$ at its output 80C, which constructs at the instant t the final filtered image.

In a variant of the method, the strings may be 2 or 3 points width instead of purely one point width as described above. In this case, the operations above-described for the one point-wide string are applied on all points constituting the several point-wide strings. In any case, the string structure looks like a regular ribbon instead of the original irregular threadlike structure that is the original image of the guide-wire above-described as example.

Referring to FIG.4A, image data of an image sequence, provided for instance by a medical examination apparatus 150, is further provided to an image processing system 120 for processing the data according to the above-cited method. This image processing system 120 may be a suitably programmed computer, a processor of a workstation 130, or a

special purpose processor having circuit means such as LUTs, Memories, Filters, Logic Operators, that are arranged to perform the functions of the method steps according to the invention. The workstation 130 may also comprise a keyboard 131, a screen 140 and a mouse 132. The processing system may be connected to storing means to store the medical images.

5 Referring to FIG.4B, an X-ray medical examination apparatus 150 comprises means for acquiring digital medical image data of a sequence of images at least comprising a causal and a present images, and a digital processing system 120 for processing these data according to the processing method described above. The X-ray apparatus comprises an X-ray source 101, a table 102 for receiving a patient to be examined, an optical system 103, 104
10 for providing image data to the processing system 120 which has at least one output 106 to provide image data to display and/or storage means 107. The display and storage means may respectively be the screen 140 and the memory of a workstation 130 as described in relation to FIG.4A. Said storing means may be alternately external storing means.

CLAIMS:

1. An image processing method for noise filtering an image sequence representing a threadlike structure on a background, including an acquisition of point data in first and second sequence images and an estimation of the corresponding filtered point data for constructing a filtered second image, the point data being the intensities associated to co-ordinates of image points, said method comprising, performed in each sequence image, steps of:

extracting the threadlike structure points, forming strings from said extracted points, temporally filtering the data of the points located outside the strings denoted background points, spatially filtering the data of the string points,

and constructing the filtered second image data by performing an insertion of the spatially filtered data of the string points into the temporally filtered data of the background points.

2. A method as claimed in Claim 1, comprising steps of :

based on the string formation performed in said sequence images, providing a binary control signal $[St(i,j)]$ formed of a list of the string points with their running number on the strings and their co-ordinates in the processed image, which determines whether the current point is a string point or a non-string point regarded as a background point.

3. A method as claimed in Claim 2, comprising, for constructing the filtered second image, steps of :

supplying said binary control signal $(St(i,j))$ for controlling the insertion of the spatially filtered data of the string points into the temporally filtered data of the background points.

4. A method as claimed in Claim 3, comprising, for eliminating phantom artifacts due to temporal filtering of the background data, steps of :

delivering the binary control signal $[St(i,j)]$ for controlling the insertion operation through a logic OR operation, whose inputs are the first and the second control

binary signals related to the first and the second sequence images, said OR operation triggering the spatially filtered data when at least one of the two binary control signals corresponds to a string point.

5 5. A method as claimed in Claim 4, including a spatial filtering operation performed on string point data, comprising steps of :

selecting string points $[A(i,j)]$ using the list of the control signal $[St(i,j)]$,
propagating on one string from its start point to its end point, according to the running number on the string,

10 while propagating, performing a spatial filtering on each point of the string in a causal then in an anti-causal direction as using a temporal filtering technique,
and constructing a filtered second image data by performing an insertion of the spatially filtered data of the string points into the temporally filtered data of the background points, controlled by the binary control signal.

15 6. A method as claimed in Claim 5, comprising for enhancing the string point data, steps of :

selecting of a string point $[A(i,j)]$ using the list of the control signal $[St(i,j)]$,
said string point having a spatially filtered intensity $[U(i,j)]$, forming a neighborhood (V) for
20 said string point using background points having temporally filtered intensities and
estimating a mean temporally filtered intensity in said neighborhood $[\bar{U}(V)]$;
estimating the local contrast $[LC(i,j)]$ related to said string point as a
difference between said mean intensity in said neighborhood and the intensity of said string
point and multiplying said contrast by a factor (C) for providing an enhanced contrast
25 $[C.LC(i,j)]$;

and calculating the enhanced string point intensity $[Ft(i,j)]$ as the difference
between the enhanced contrast and the mean intensity $[\bar{U}(V)]$ in the neighborhood (V) of said
point.

30 7. A method as claimed in one of Claims 5 or 6, including an enhancement operation performed on spatially filtered string point data, comprising steps of :

selecting string points $[A(i,j)]$ using the list of the control signal $[St(i,j)]$,
enhancing the string point data with respect to their local environment,

and constructing a filtered second image data by performing an insertion of the enhanced spatially filtered data of the string points into the temporally filtered data of the background points, controlled by the binary control signal.

5 8. A method as claimed in one of the preceding Claims, wherein the images are medical examination digital images and the threadlike structure is a catheter guide-wire.

9. A system comprising a suitably programmed computer of a workstation or a
10 special purpose processor having circuit means, which are arranged to process image data according to the method as claimed in any of Claims 1 to 8, and having means to display images processed according to said method, and possible means to store the image data.

10. An X-ray apparatus having means for acquiring medical digital image data and
15 having a system as claimed in claim 9 having access to said medical digital image data for processing said image data.

11. A computer program product comprising a set of instruction for carrying out a method as claimed in one of claims 1 to 8.

ABSTRACT:

The invention relates to an image processing method for noise filtering an image sequence representing a threadlike structure on a background, including an acquisition of point data in first and second sequence images and an estimation of the corresponding filtered point data for constructing a filtered second image, said method comprising,

5 performed in each sequence image, steps of:

extracting the threadlike structure points, forming strings from said extracted points, temporally filtering the data of the points located outside the strings denoted background points, spatially filtering the data of the string points,

10 and constructing the filtered second image data by performing an insertion of the spatially filtered data of the string points into the temporally filtered data of the background points.

In an application, the sequence images are X-ray fluoroscopic images representing a catheter guide-wire. The invention also relates to a system and an X-ray apparatus for carrying out the method.

15 FIG.1.

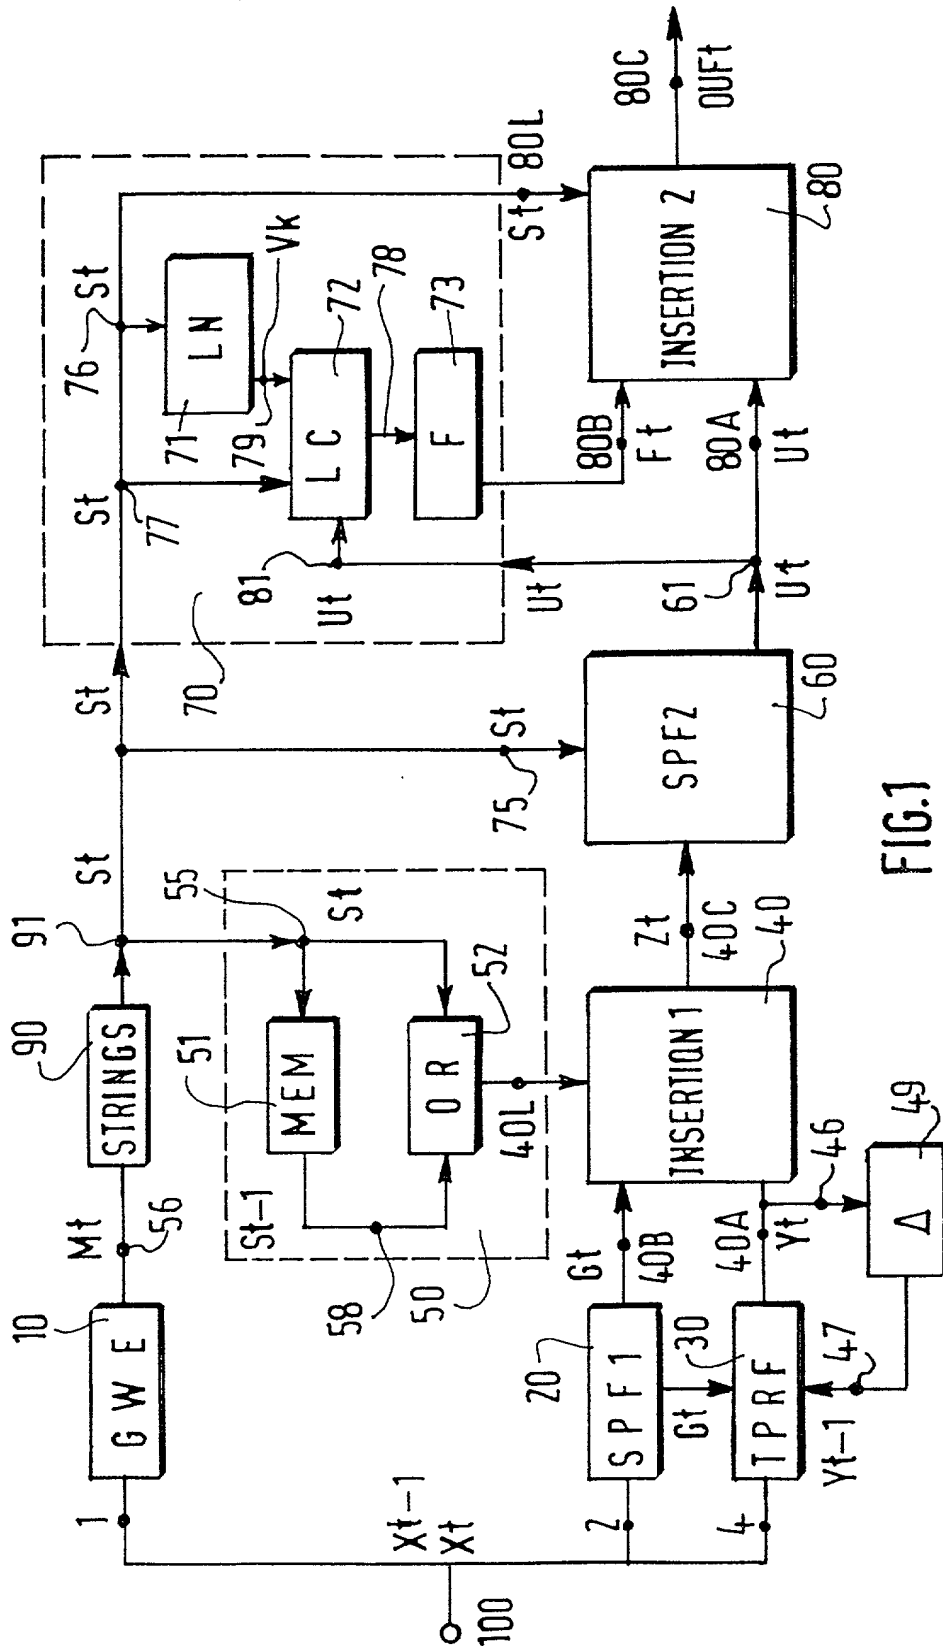


FIG. 1

2/3

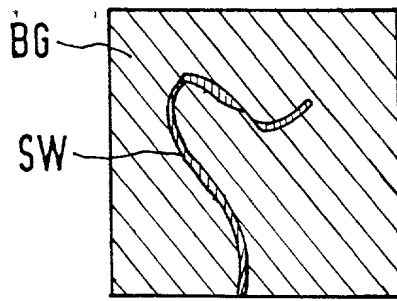


FIG. 2A

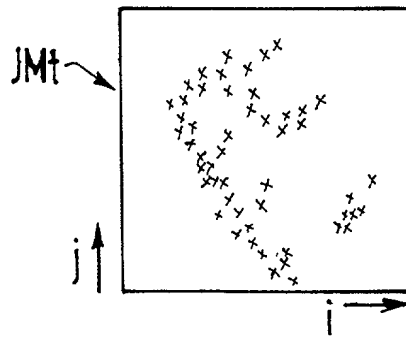


FIG. 2B

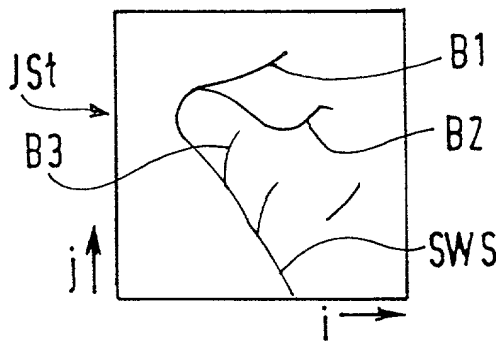


FIG. 2C

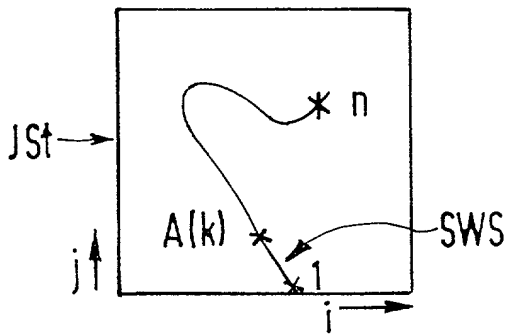


FIG. 2D

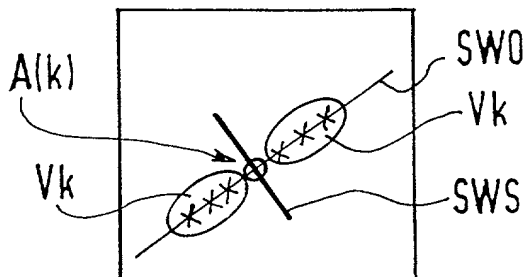


FIG. 3

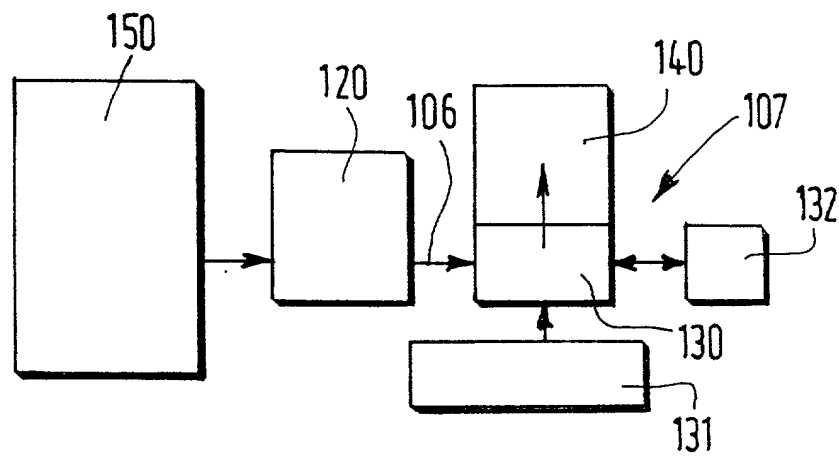


FIG. 4A

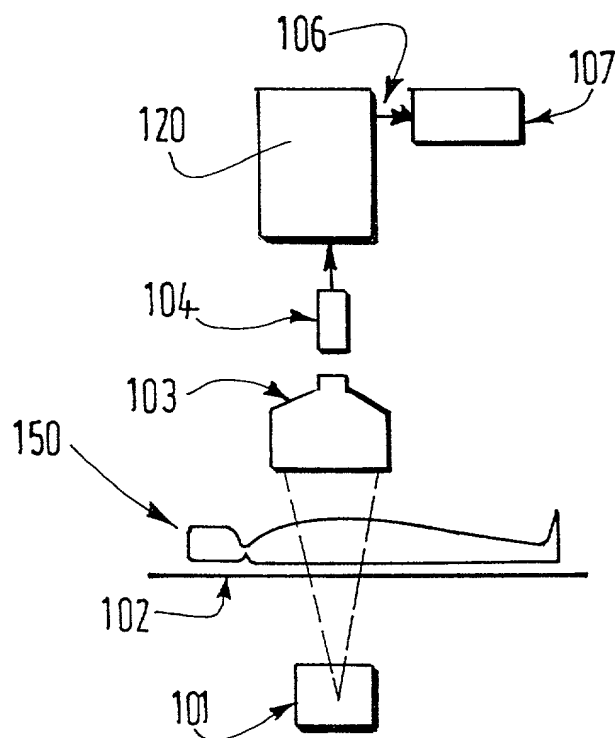


FIG. 4B

DECLARATION and POWER OF ATTORNEY

ATTORNEY'S DOCKET NO.:

PHF 99.595 US

As a below named inventor, I hereby declare that:

My residence, post office address and citizenship are as stated below next to my name.

I believe I am the original, first and sole inventor (if only one name is listed below) or an original, first joint inventor (if plural names are listed below) of the subject matter which is claimed and for which a patent is sought on the invention entitled

"Image processing method, system and apparatus for noise reduction in an image sequence representing a threadlike structure"

the specification of which (check one)

☐ is attached hereto.☐ was filed on _____ as Application Serial No. _____ and was amended on _____ (if applicable).

I hereby state that I have reviewed and understand the contents of the above-identified specification, including the claims, as amended by the amendment(s) referred to above.

I acknowledge the duty to disclose information which is material to patentability of this application in accordance with Title 37, Code of Federal Regulations, §1.56(a).

I hereby claim foreign priority benefits under Title 35, United States Code, § 119 of any foreign application(s) for patent or inventor's certificate listed below and have also identified below any foreign application for patent or inventor's certificate having a filing date before that of the application on which priority is claimed:

PRIOR FOREIGN APPLICATION(S)

COUNTRY	APP. NUMBER	DATE OF FILING (DATE, MONTH, YEAR)	PRIORITY CLAIMED UNDER 35 U.S.C. 119
Europe	99402662.3	26 October 1999	YES

I hereby claim the benefit under Title 35, United States Code, §120 of any United States application(s) listed below and, insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States application in the manner provided by the first paragraph of Title 35 United States Code, §112, I acknowledge the duty to disclose material information as defined in Title 37, Code of Federal Regulations, §1.56(a) which occurred between the filing date of the prior application and the national or PCT international filing date of this application:

PRIOR UNITED STATES APPLICATION(S)

APPLICATION SERIAL NUMBER	FILING DATE	STATUS (PATENTED, PENDING, ABANDONED)

I hereby declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code and that such willful false statements may jeopardize the validity of the application or any patent issued thereon.

POWER OF ATTORNEY: As a named inventor, I hereby appoint the following attorney(s) and/or agent(s) to prosecute this application and transact all business in the Patent and Trademark Office connected therewith. (list name and registration number)

Jack E. Haken, Reg. No. 26,902
Michael E. Marion, Reg. No. 32,266
Edward M. Blocker, Reg. No. 30,245

SEND CORRESPONDENCE TO: Corporate Patent Counsel;
U.S. Philips Corporation;
580 white Plains Road; Tarrytown, NY 10591

DIRECT TELEPHONE CALLS TO:
(name and telephone No.)
(914) 332-0222

Dated:		Inventor's Signature:	
Full Name of in Inventor	Last Name FLORENT	First Name Raoul	Middle Name
Residence & Citizenship	City Vlenton	State of Foreign Country France	Country of Citizenship France
Post Office Address	Street 1 Chemin des Aulnettes	City 94460 Valenton	State of Country France
Zip Code			
Dated:		Inventor's Signature:	
Full Name of in Inventor	Last Name GOUBET	First Name Lucile	Middle Name
Residence & Citizenship	City Paris	State of Foreign Country France	Country of Citizenship France
Post Office Address	Street 5 rue de la Voûte	City 75012 Paris	State of Country France
Zip Code			

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re Application of
RAOUL FLORENT et al.

Atty. Docket
PHF 99,595



Filed: CONCURRENTLY

IMAGE PROCESSING METHOD, SYSTEM AND APPARATUS FOR NOISE REDUCTION IN
AN IMAGE SEQUENCE REPRESENTING A THREADLIKE STRUCTURE

Commissioner for Patents, Washington, D.C. 20231

APPOINTMENT OF ASSOCIATES

Sir:

The undersigned Attorney of Record hereby revokes all
prior appointments (if any) of Associate Attorney(s) or Agent(s) in
the above-captioned case and appoints:

JOHN F. VODOPIA

Reg. 36,299

c/o U.S. PHILIPS CORPORATION, Intellectual Property Department, 580
White Plains Road, Tarrytown, New York 10591, his Associate
Attorney(s)/Agent(s) with all the usual powers to prosecute the above-
identified application and any division or continuation thereof, to
make alterations and amendments therein, and to transact all business
in the Patent and Trademark Office connected therewith.


ALL CORRESPONDENCE CONCERNING THIS APPLICATION AND THE
LETTERS PATENT WHEN GRANTED SHOULD BE ADDRESSED TO THE UNDERSIGNED
ATTORNEY OF RECORD.

Respectfully,

Michael E. Marion, Reg. 32,266
Attorney of Record

Dated at Tarrytown, New York
on 18TH October, 2000.

United States Patent & Trademark Office
Office of Initial Patent Examination -- Scanning Division

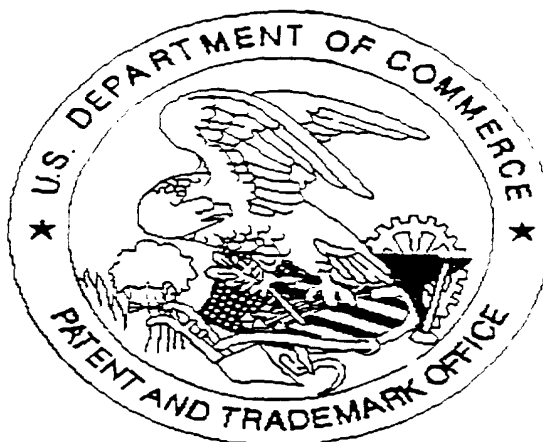

Application deficiencies were found during scanning:

☐ Page(s) _____ of _____ were not present:
for scanning. (Document title)

☐ Page(s) _____ of _____ were not present:
for scanning. (Document title)

There is one sheet of declaration.

☐ Scanned copy is best available.